

QuaTest FTMS Rapid Test Kit

(Florfenicol & Thiamphenicol / Trimethoprim / Meloxicam / Sulfonamides)

Art. No.: 100052-96T

Principle

This product utilizes the high affinity antibodies and capture protein against meloxicam, trimethoprim, sulfonamides, thiamphenicol and florfenicol antibiotics, which can easily identify these potential hazardous substances in milk without any instrument.

1. Detection Limit (LOD) in Raw milk sample

Thiamphenicol	LOD(µg/L)	Florfenicol	LOD(µg/L)
Thiamphenicol	1-2	Florfenicol	0.8-1
Trimethoprim	LOD(µg/L)	Meloxicam	LOD(µg/L)
Trimethoprim	0.5-1	Meloxicam	1.5-2
Sulfonamides	LOD(µg/L)	Sulfonamides	LOD(µg/L)
Sulfachlorpyridazine	5-7	Sulfathiazole	60-80
Sulfadiazine	5-8	Sulfamonomethoxine	3-4
Sulfadoxine	3	Sulfamoxole	20-30
Sulfamerazine	4-6	Sulfadimidine	5-8
Sulfamethizole	4-6	Sulfisomidine	2-4
Sulfamethoxazole	6-10	Sulfachloropyrazine	4-6
Sulfamethoxy pyridazine	8-10	Sulfamethoxydiazine	3-4
Sulfapyridine	60-90	Sulfisoxazole	40-60
Sulfaquinoxaline	5-8	Sulfadimethoxine	2-4

2. Kit components

- Test Strip: 96 pcs / package.
- Kit instruction

3. Operations

- Read the instructions before experiment. Bring the test kit and samples to room temperature. Milk samples should be fully liquid without any agglomeration and deposition.
- Take out required wells and strips from the package, and make proper marks. Please use the test strips within 1h. Seal the cap of the bottles and store the rest of the unused kit.
- Take 200ul of the milk sample into the microwell, then repeatedly absorb up and down for 5 times to mix the sample with the reagent in the wells completely. The mixture should be pink, and then start the timer.

Note: In case you are sampling with plastic pipet, please add sample to the MARKER LINE on the microwell.

- Incubate for **3min at room temperature**, and then insert the test strip into the well with the "Immersed" end fully dipped in to the mixed reagent and sample.
- Incubate for **7min at room temperature**. Take out the strip; determine the result according to **Part 4**.

4. Result Determination

There are 5 lines on the strip, **Control line, Thiamphenicol/Florfenicol Line, Trimethoprim Line, Meloxicam Line and Sulfonamides Line**, which are briefly used as "**Line C**", "**Line T1**", "**Line T2**", "**Line T3**" and "**Line T4**". The test results will depend on the color of these lines. The following diagram describes the result determination.

INVALID

Line C has no color. **In this case, the test will be invalid.**

NEGATIVE

Thiamphenicol/Florfenicol Negative: Compare the color of Line T1 with Line C, if the color of Line T1 **is**

deeper than Line C, the result will be **negative**.

Trimethoprim Negative: Compare the color of Line T2 with Line C, if the color of Line T2 is deeper than Line C, the result will be **negative**.

Meloxicam Negative: Compare the color of Line T3 with Line C, if the color of Line T3 is deeper than Line C, the result will be **negative**.

Sulfonamides Negative: Compare the color of Line T4 with Line C, if the color of Line T4 is deeper than Line C, the result will be **negative**.

POSITIVE

Thiamphenicol/Florfenicol Positive: Compare the color of Line T1 with Line C, if the color of Line T1 is lighter than or the same as Line C, the result will be **positive**, if there is no Line T1, the result is also **positive**.

Trimethoprim Positive: Compare the color of Line T2 with Line C, if the color of Line T2 is lighter than or The same as Line C, the result will be positive. If there is no Line T2, the result is also **positive**.

Meloxicam Positive: Compare the color of Line T3 with Line C, if the color of Line T3 is lighter than or The same as Line C, the result will be positive. If there is no Line T3, the result is also **positive**.

Sulfonamides Positive: Compare the color of Line T4 with Line C, if the color of Line T4 is lighter than or The same as Line C, the result will be positive. If there is no Line T4, the result is also **positive**.

PLEASE NOTICE Line C is used as a quality indicator, which will always appear regardless of the T1/T2/T3/T4 line. If Control line does **NOT** appear, this indicates that the result is **invalid**. Users please check the kit insert again and repeat the assay with new test strip.

5. Storage

2-8°C in cool dark place, do not freeze. The kit is valid for 12 months after manufacture date. Lot number and expired date are printed on the package.


6. Notice and Precautions for a successful experiment.

Please perform the assay following the instruction, do not touch the membrane of the strip.

Please seal the bottle after taking out required strips.


This strip is used for only once; please do not use it repeatedly.

This kit is only for screening test, positive result should be further confirmed with other method.


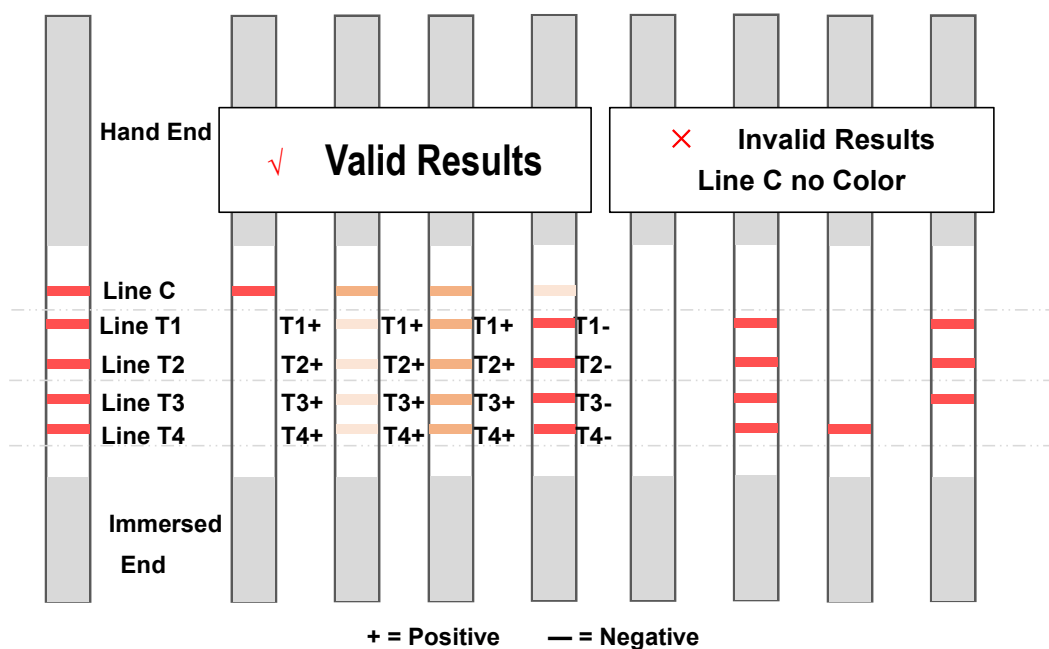


Schematic Assay Steps


1. Bring all test samples to room temperature; number them to keep record.




2. Take test kit according to your sample number and also number the kit wells to keep record and consistency.

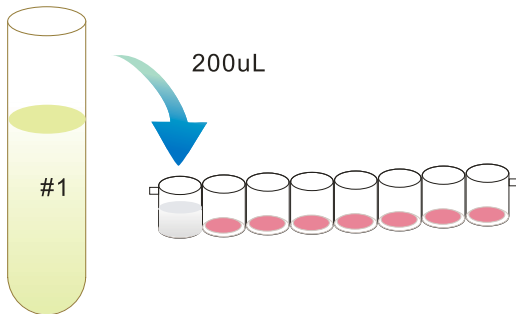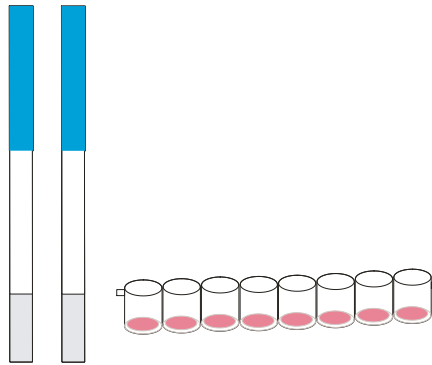


3. Take 200ul sample into the wells using pipet. You can also then put the well into the well holder to avoid sample spill.

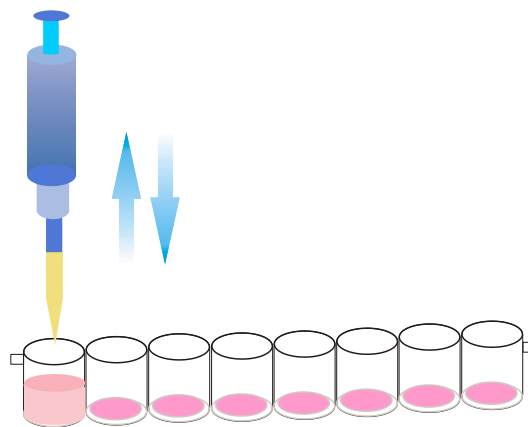

4. Absorb up and down for 5 times to mix sample with reagent completely. Start the timer when the mixture is pink. **Incubate for 3 min.**

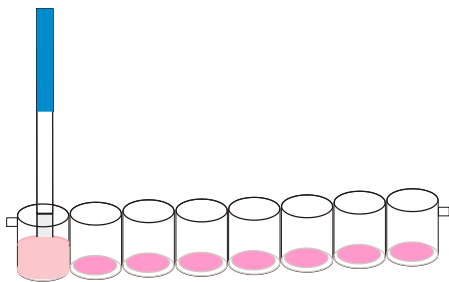

5. Insert the "Immersed" end of the strip into the mixture; **Incubate for 7 min at room temperature again.**

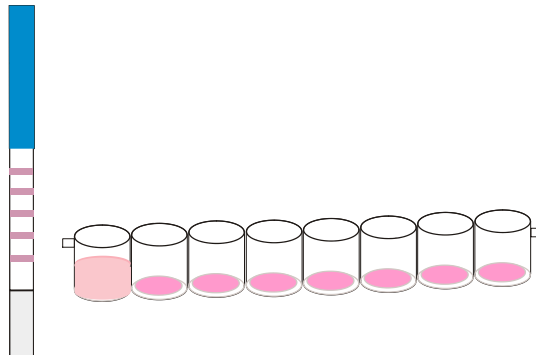

6. Take out the strip; judge the result according to **kit instruction.**

Ring Biotechnology Co., Ltd

Add: Building 3, Zhongtongtai TechnoPark, No. 11, Kechuang 14th St, Beijing 100176, CHINA

E-mail: info@ringbio.com Web: www.ringbio.com Tel: +86-10-56267496